




Surgical Report

Order Details

APPROVED

Patient Name: 우즈벡-37
Client Order Reference: 93991_20240424_1043_06
Creation Date: 2024-04-25 오후 5:33:42
Approved by: Default user
 (940d2431-9248-4915-869e-86f305364413)

하악




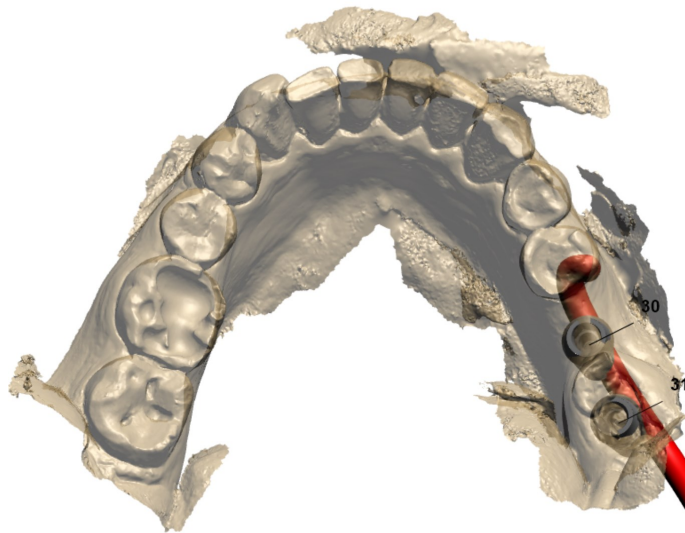


Implant information		
Implant position (UNN)	30	31
제조업체	YESBIOTECH	YESBIOTECH
Type	MY-Q Implant 5mm x 10mm, P5.0	MY-Q Implant 5mm x 10mm, P5.0
Order number	BB5010573	BB5010573
Length, mm	10	10
Diameter (Ø), mm	5	5
Color	Blue	Blue

Limitation of Liability:

This instruction incorporates a custom document that is based on a surgical plan proposed by the surgeon before operation. The surgeon, therefore, takes full medical responsibility for the design and the application of the surgical guide, the intended used surgical tray kit, implants and sleeves – all as specified on the order form received by the supplier. The custom document shall be considered as an addition to all other documents sent with and pertaining to the case, and it does not replace any of those other documents.




Implant Information	
Implant position (UNN)	30
제조업체	YESBIOTECH
Type	MY-Q Implant 5mm x 10mm, P5.0
Order number	BB5010573
Length, mm	10
Diameter (Ø), mm	5
Color	Blue
Safety zone - apical distance	2.0
Safety zone - radial distance	1.5

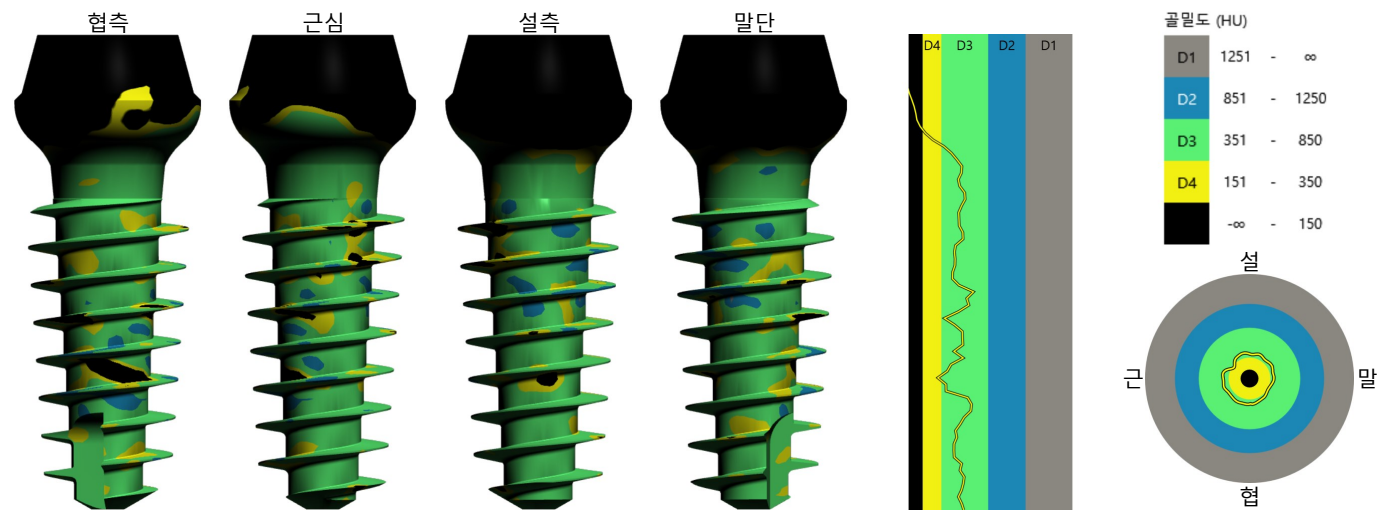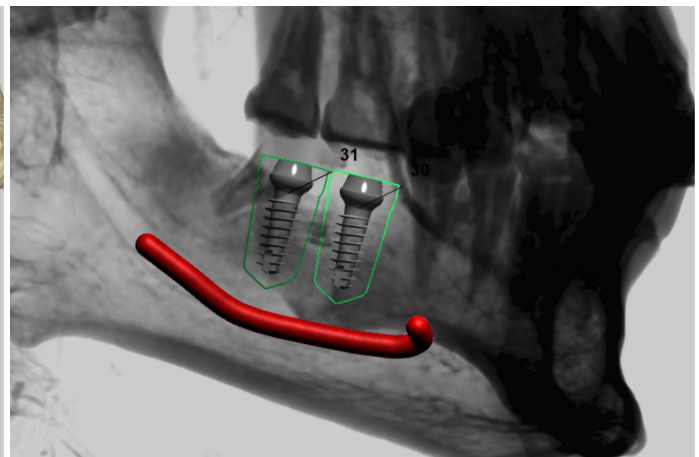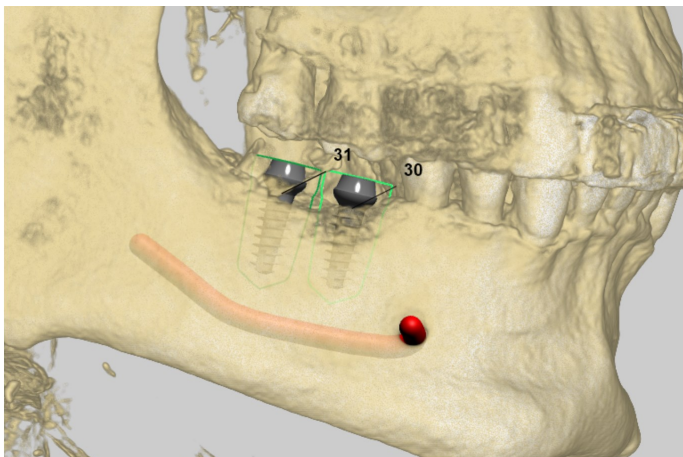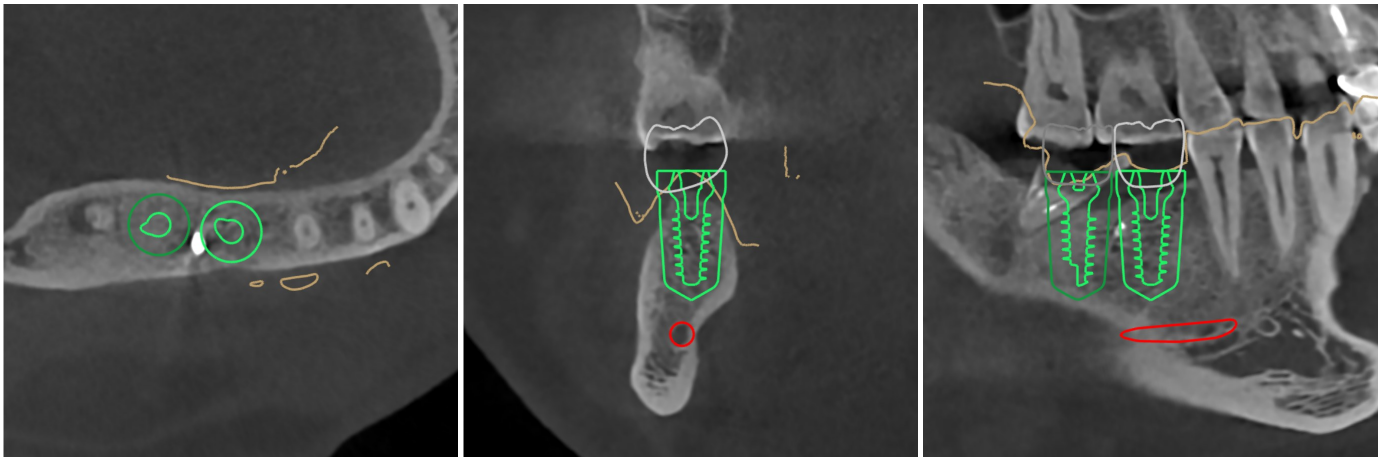

Limitation of Liability:

This instruction incorporates a custom document that is based on a surgical plan proposed by the surgeon before operation. The surgeon, therefore, takes full medical responsibility for the design and the application of the surgical guide, the intended used surgical tray kit, implants and sleeves – all as specified on the order form received by the supplier. The custom document shall be considered as an addition to all other documents sent with and pertaining to the case, and it does not replace any of those other documents.

Implant Information	
Implant position (UNN)	31
제조업체	YESBIOTECH
Type	MY-Q Implant 5mm x 10mm, P5.0
Order number	BB5010573
Length, mm	10
Diameter (Ø), mm	5
Color	Blue
Safety zone - apical distance	2.0
Safety zone - radial distance	1.5

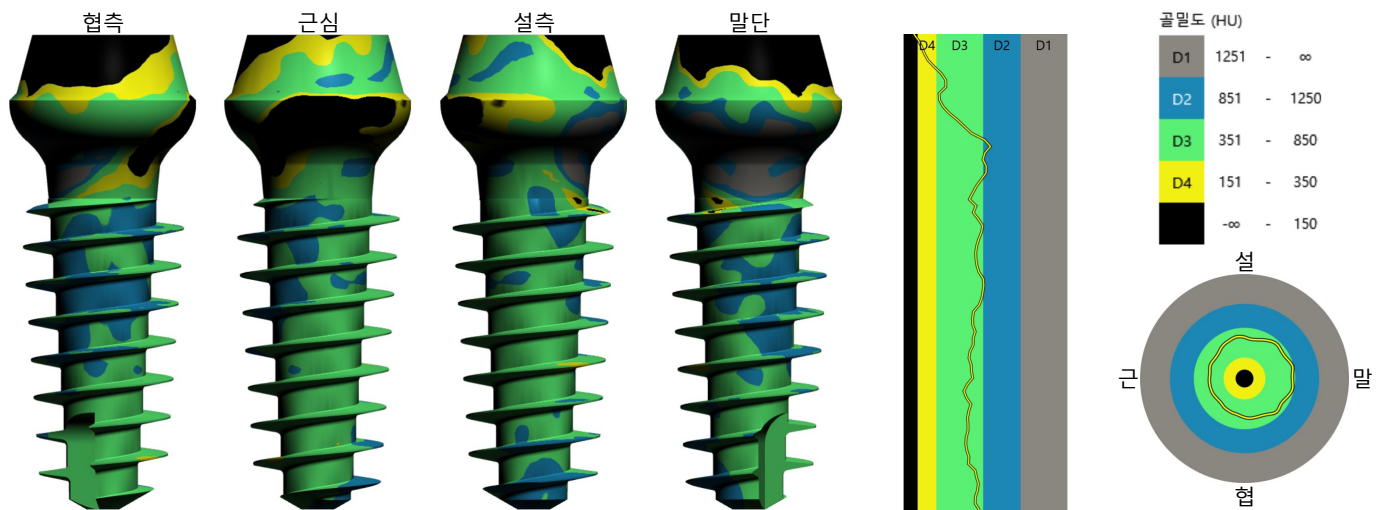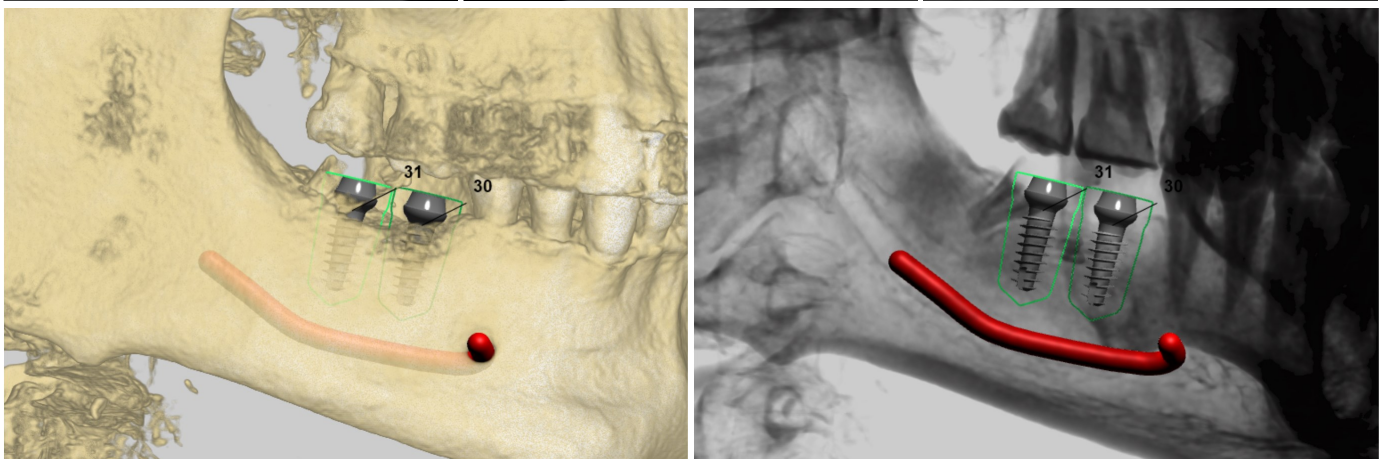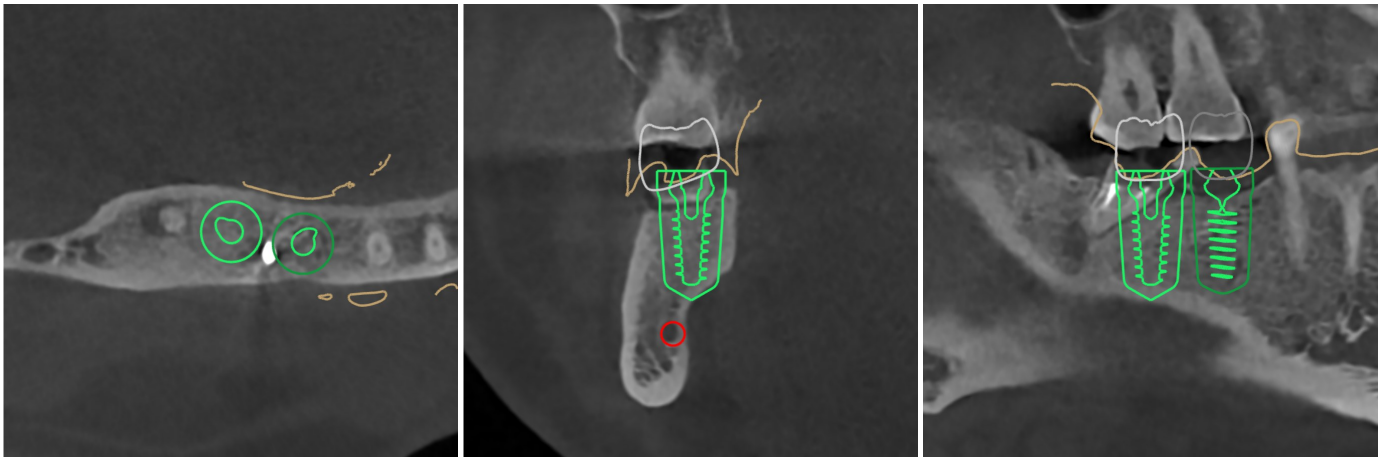

Limitation of Liability:

This instruction incorporates a custom document that is based on a surgical plan proposed by the surgeon before operation. The surgeon, therefore, takes full medical responsibility for the design and the application of the surgical guide, the intended used surgical tray kit, implants and sleeves – all as specified on the order form received by the supplier. The custom document shall be considered as an addition to all other documents sent with and pertaining to the case, and it does not replace any of those other documents.